



PRODUCT CATALOGUE

BIG IN POLISHING
HUGE IN QUALITY




ORDER ONLINE



Please check out the mobile website with all products and descriptions:

<http://m.kenda-dental.com>

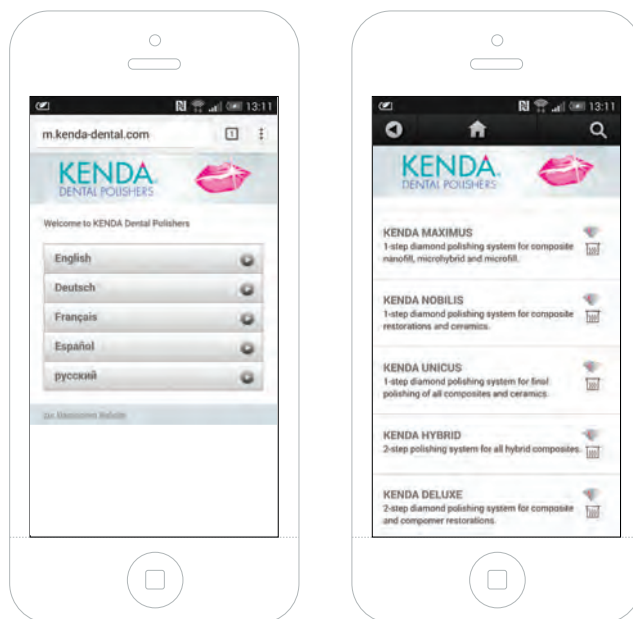

For the catalogue
in PDF
in English



<http://knd.li/eng>



ORDER ONLINE



<http://knd.li/shp>

ABOUT KENDA


KENDA = POLISHING RESOLVED

In 1977 the world was a different place. Jimmy Carter was President of the United States, the first Star Wars movie came out and in June Elvis Presley gave his last concert.

The world of dentistry, too, was quite different back then.

Microfilled composites were becoming more and more popular restoratives, replacing the dominant amalgam and macrofills bit by bit. The new material was esthetically pleasing, its color much more natural. But it was difficult to polish with the common polishers.


KENDA was founded in the same year with the aim to develop a proper solution for this problem every dentist was facing. In cooperation with Professor Whitehead at the University of Manchester's Dental School, newly founded **KENDA** developed the most optimized polishing system for microfilled composites available at the time and struck a chord in the dental community.

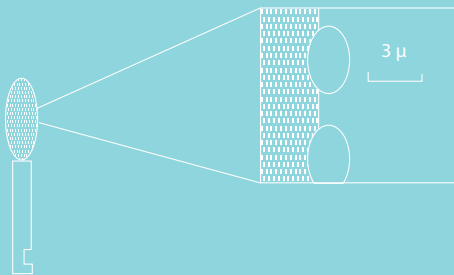

The KENDA 3 - Micron Silicone Point
An Initial Evaluation
S.A. Whitehead

Now, over 40 years later **KENDA** is a global leader in dental polishing solutions. The road from 1977 into the present is marked by industry milestones. In 1991, **KENDA** Hybrid, the first diamond polisher for intraoral use on hybrid composites was introduced. This invention put an instrument into dentists' hands which enabled them to achieve high shine results on a material it was believed to remain impossible. Ten years after **KENDA** Hybrid, the **KENDA** Nobilis 1-step polishers rose to fame, reducing polishing time for the dentist dramatically.

Since the beginning, the constant adapting to the polishing requirements of dentists and the continuously improved restoratives has never stopped for **KENDA**. In the past, today and in the future it will be **KENDA**'s mission to provide the dental community with the newest polishing technology at the highest quality. Currently the dentists' focus is shifting more and more on infection control and streamlining work processes. Consequently, single-use polishing is becoming ever more popular, for which **KENDA** is offering one of the most advanced solutions today: the Polishettes®. Also the increasing use of CAD/CAM milling directly in the dental office promotes the diffusion of high end ceramics such as Zirconia. The **KENDA** Zircovis polishing solution provides the right tool for the dentist to master the reduction of surface roughness and the restoration of gloss after intra-oral adjustment of these extremely hard materials.

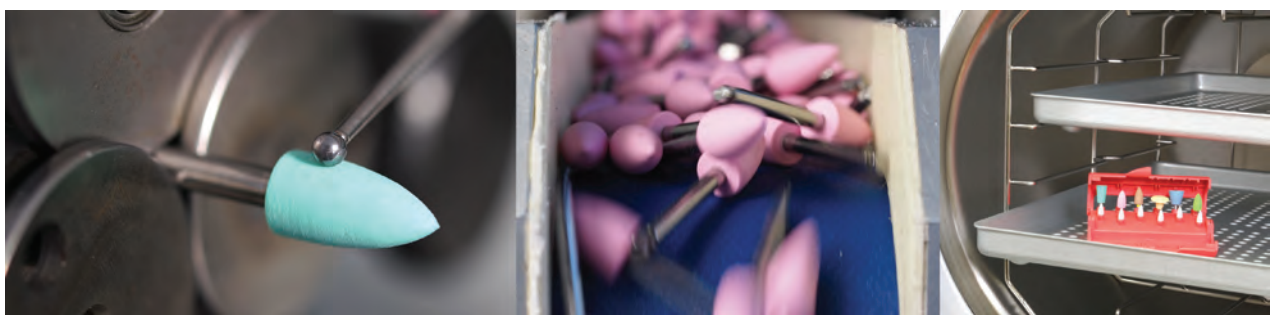

ABOUT KENDA



WE ARE LIVING AND BREATHING POLISHERS SINCE 1977

For us, it's all about polishers.


Our history in the development and production of dental polishers (and dental polishers only!) equips us with an experience and focus second to none. That is the rock-solid base from which we develop new products. Tailored to whatever your restorative situation or preference may be.




WE THOROUGHLY WATCH OUR DEVELOPMENT PROCESS

Our performance analysis for new products comprises quantitative and qualitative methods.

Surface roughness tests

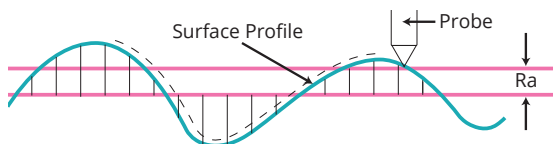

Gloss Measurement

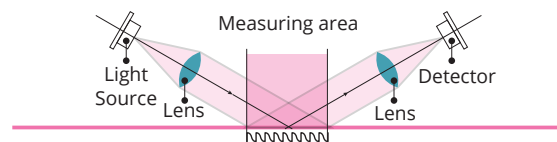

WE CAREFULLY SELECT OUR RAW MATERIALS

We pay particular attention to the abrasives and matrix materials we mold into the final product. Abrasive particles all have their unique characteristics with different effects on the surface. A small deviation in the raw material can have a large impact on the result.



WE CONDUCT 100% FINAL VISUAL INSPECTION

Numerous in-process and final quality checks are performed on the polishers: sample destructive testing of every batch produced and various non-destructive tests. And in the end, each and every polisher is visually checked by a human before being packaged.



WE ARE ISO CERTIFIED SINCE 1996

We strictly adhere to the ISO 13485 standard and comply with 93/42 EEC. We hold the CE mark for medical class IIa devices and all of our products are FDA compliant.



WE KEEP TRACK

All of our packages are labeled with LOT number and barcode. This allows us to trace back simply everything along the supply chain.












WE CUSTOM-BRAND YOUR POLISHERS

We are an experienced manufacturer of Private Label polishing solutions. With all development knowledge and technology in-house, we can furnish your new polishing line according to your needs quickly.




TABLE OF CONTENTS

CLINICAL RA - STEEL SHANK MULTI - USE

PAGE	PRODUCT	APPLICATION	FLEXIBILITY
MULTIPLE MATERIALS			
9	 KENDA NOBILIS	For Composites, Porcelain & Hybrid-Ceramics	Flexible
10	 KENDA UNICUS	For Composites, Porcelain & Hybrid-Ceramics	Flexible
11	KENDA COMPLETE	For Composites, Compomers, Amalgam & Gold	Flexible
COMPOSITES			
12	 KENDA MAXIMUS	For All Composites & Hybrid-Ceramics	Flexible
13	 KENDA DELUXE	For All Composites, Compomers & Hybrid-Ceramics	Flexible
14	 KENDA HYBRID	Optimized For Hybrid Composites	Hard
15	KENDA MICROFILL	Optimized For Microfilled Composites; Removing of Cement Remnants	Flexible
16	KENDA C.G.I.	For Universal Composites, Compomers & Glass-Ionomers	Flexible
CERAMICS			
17	 KENDA ZIRCO I	For All Oxide & Silicate Ceramics - Optimized For Zirconia	Hard
18	 KENDA ZIRCOVIS	For All Oxide & Silicate Ceramics - Optimized For Zirconia	Hard
19	 KENDA ALL CERAMIC	For All Oxide & Silicate Ceramics	Flexible
ENAMEL			
20	KENDA PROPHY	Tooth Cleaning & Removal of Extrinsic Stains without Polishing Paste	Flexible
ACRYLICS			
21	KENDA PLANUS	For Acrylic Dentures, Retainers, Mouth Guards and Snoring Mouth Pieces	Flexible
AMALGAM AND METALS			
22	KENDA AMALGAM	For Amalgam & Precious Metals	Flexible
23	 KENDA PRECIOUS METALS	For Titanium Alloys, Precious & Non-Precious Metals	Hard

4

CLINICAL RA - PLASTIC SHANK DISPOSABLE

PAGE	PRODUCT	APPLICATION	FLEXIBILITY
COMPOSITES			
25	 POLISHETTE 	For Composites & Hybrid-Ceramics	Flexible
26	 DISPOSABLE KENDA G.P.S.	For Composites, Compomers & Hybrid-Ceramics	Flexible
27	DISPOSABLE KENDA BIG JOB	For All Composites	Flexible

CLINICAL FG - STEEL SHANK MULTI - USE


PAGE	PRODUCT	APPLICATION	FLEXIBILITY
MULTIPLE MATERIALS			
29	 KENDA 0306FG/0386FG	For Composites & Porcelain - On Friction Grip Shank	Hard
COMPOSITES			
29	KENDA 4006FG/5006FG	For All Composites - On Friction Grip Shank	Hard
AMALGAM AND METALS			
29	KENDA 2006FG/3006FG	For Amalgam and Precious Metals - On Friction Grip Shank	Hard



Grit size range specified for each step according to ISO guidelines. Cutting properties of the same grit size vary depending on the shape and material of the abrasive particles.





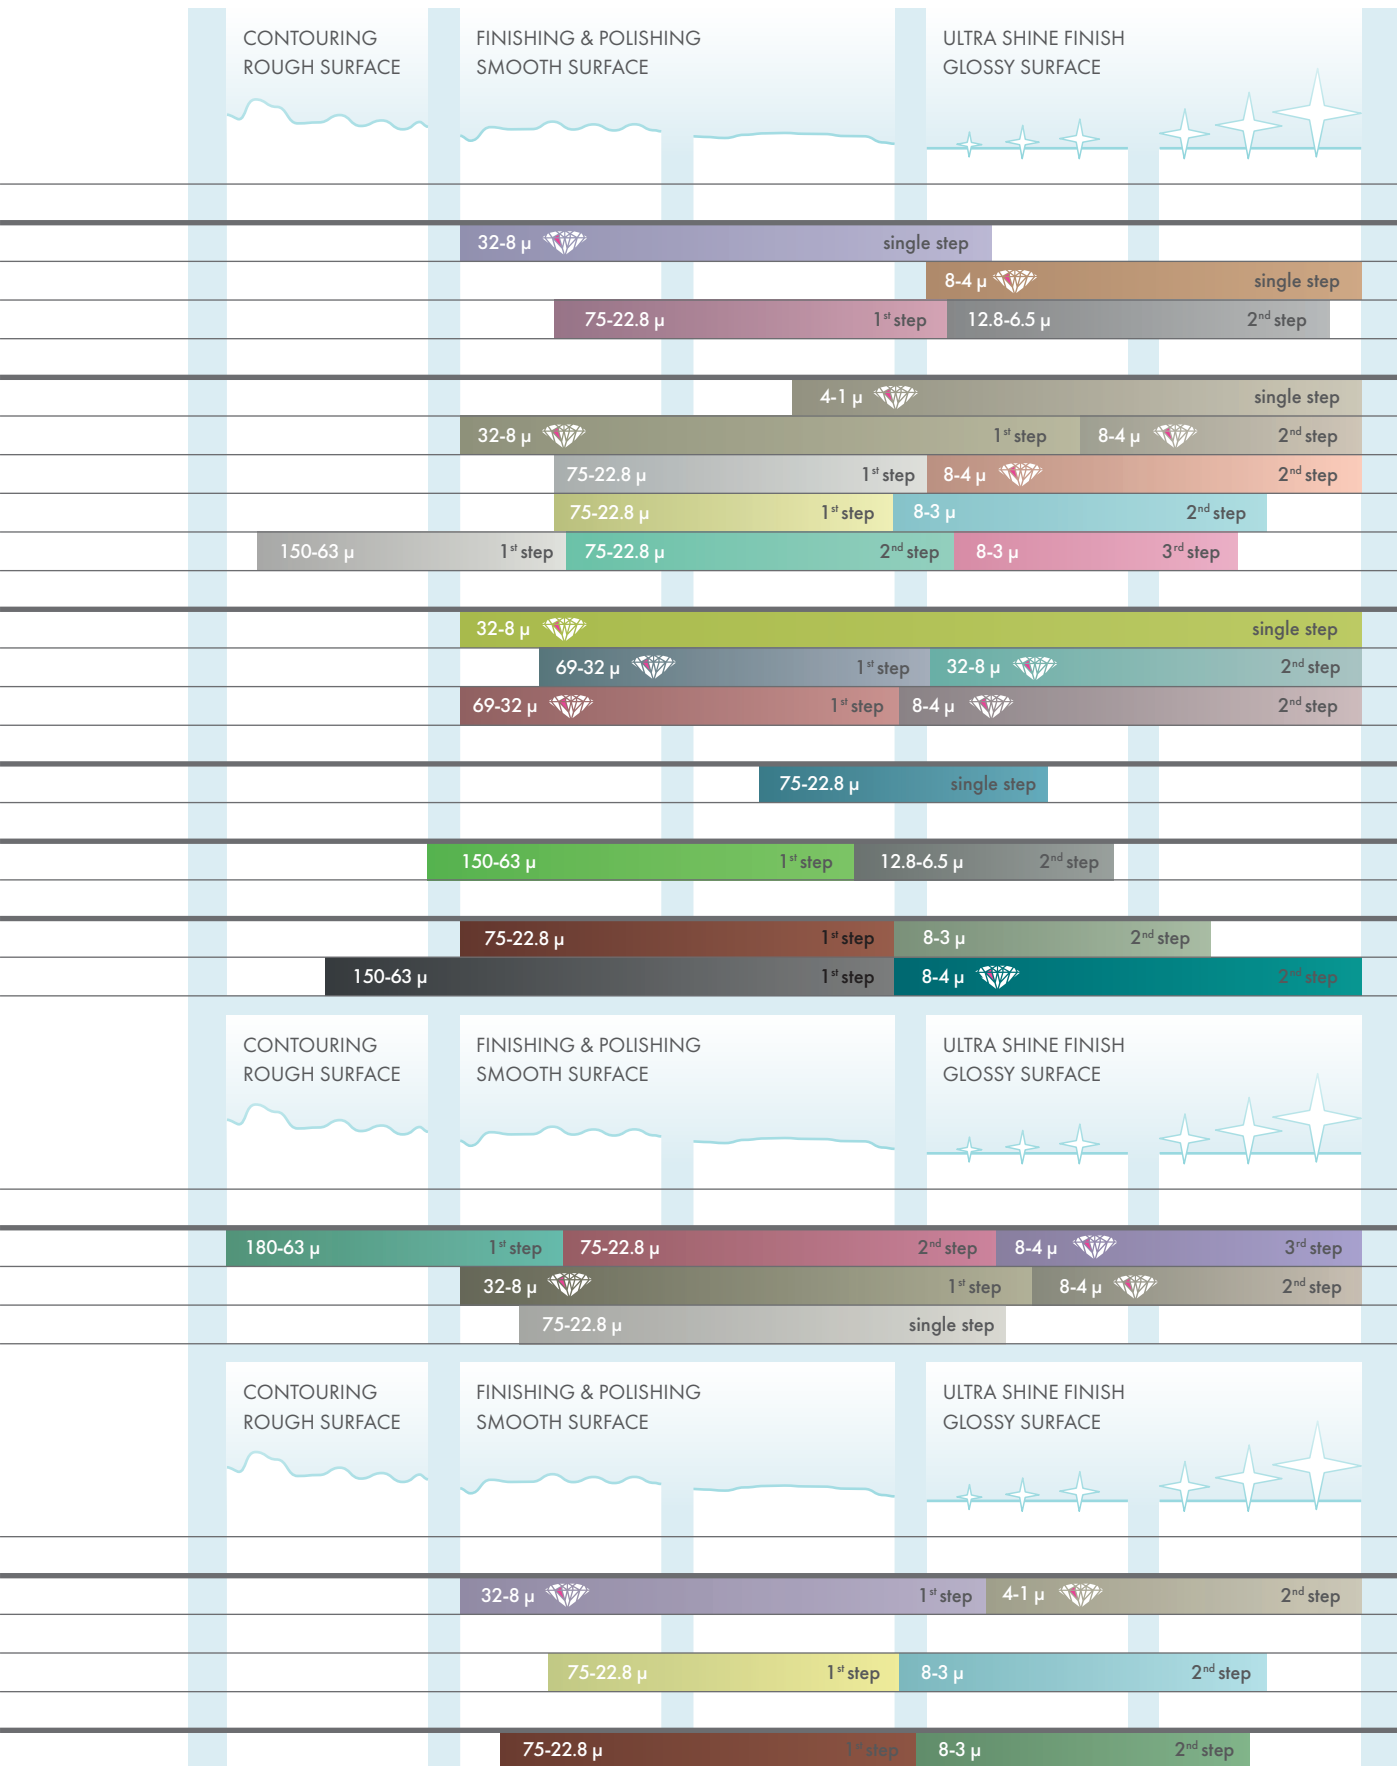

The diamond symbolizes that the specific step is diamond impregnated. Diamond polishers are the most efficient, reducing polishing time and achieving the best surface results and gloss values.



Please note that the chart is only for general orientation and facilitating product choice. Polishing results may differ depending on the specific composition of the restorative material polished. Applied pressure and rotational speed influences the polishing result. Subject to change (product enhancements). Errors and omissions excepted.

TABLE OF CONTENTS

LABORATORY

PAGE	PRODUCT	APPLICATION	FLEXIBILITY
CERAMICS			
31	 KENDA Z-SERIES	For All Types of Ceramics including Zirconia, Alumina and Lithium Disilicate	Hard
32	 KENDA HIGH END	For All Types of Ceramics including Zirconia, Alumina and Lithium Disilicate	Hard
33	KENDA W&K 6500-7500	For Silicate Ceramics	Flexible
ACRYLICS			
34	KENDA RED	For Acrylic Dentures - Optimized for Partial on Chrome Cobalt Alloys	Flexible
35	KENDA QUEEN	For Acrylic Dentures	Flexible
36	KENDA ACRYLIC BLUE	For Acrylic Dentures	Flexible
37	KENDA YELLOW LINE	Acrylic Dentures - Finishing Set	Flexible
38	KENDA PLANUS	For Acrylic Dentures, Retainers, Mouth Guards and Snoring Mouth Pieces	Flexible
FLEXIBLE DENTURES			
39	KENDA BESTFLEX	For All Nylon Based Flexible Dentures	Flexible
METALS			
40	 KENDA PRECIOUS METALS	For All Precious, Semi and Non-Precious Metals, CoCr and Titanium	Hard
41	KENDA W&K 2500-3500	For Gold and Semi-Precious Alloys	Flexible
41	KENDA W&K 9500	For Titanium	Flexible
COMPOSITES			
42	 KENDA HYBRID	For All Composite Materials	Hard
MULTIPLE MATERIALS			
33	KENDA W&K 1500	For All Alloys and Acrylic Dentures	Flexible

6

ACCESSORIES

PAGE	PRODUCT	APPLICATION
43	KENDA PRACTICUS	Autoclavable Polisher and Bur Caddy

INFORMATION

PAGE	PRODUCT
45	PACKAGING, LABEL AND SYMBOLS
49	ABOUT POLISHING AND INSTRUCTION FOR USE

CONTOURING
ROUGH SURFACE

FINISHING & POLISHING
SMOOTH SURFACE

ULTRA SHINE FINISH
GLOSSY SURFACE



164-69 μ 1st step 69-32 μ 2nd step 32-8 μ 3rd step

164-69 μ 1st step 69-32 μ 2nd step 32-8 μ 3rd step 8-4 μ 4th step

150-63 μ 1st step 75-22.8 μ 2nd step

150-63 μ single step

>150 μ 1st step 150-63 μ

>150 μ 1st step 150-63 μ 2nd step 12.8-6.5 μ 3rd step

150-63 μ single step

150-63 μ 1st step 12.8-6.5 μ 2nd step

150-63 μ single step

150-63 μ 1st step 8-4 μ 2nd step

75-22.8 μ 1st step 8-3 μ 2nd step

150-63 μ single step

75-22.8 μ 1st step 8-4 μ 2nd step


150-63 μ single step



CLINICAL

MULTI-USE POLISHERS

Polishers feature an autoclavable steel-shank and are disinfected and sterilized before and after each use. Sterilize in an autoclave at 135°C/ 275°F.



Polishers for intra-oral use on multiple patients



Consult instructions for use for detailed sterilization procedure





KENDA NOBILIS

1-STEP DIAMOND POLISHING SYSTEM


- Polish porcelain and composites with the same polisher
- For a silky luster in only 1 step
- Economical diamond polisher ideal for posterior restorations
- Flexible, adapting to tooth shape
- Recommendation: For anterior restorations, use KENDA Maximus or KENDA Unicus polishers subsequently for ultimate high shine polishing



SET REF 0300.006A



REF reorder	0301	0302	0303	0305	0306	0308	0309	0310	0311
ISO 1: 858 204...	243 513 055	254 513 050	304 513 100	030 513 060	243 513 030	243 513 050	303 513 100	030 513 090	030 513 060
$\varnothing \times L$ mm	5,4 x 13	5 x 8	10 x 2	6,5 x 10	3 x 7	5 x 10	10 x 1	9 x 8,5	6 x 7,5
μ grit	fine		μ grit		color		rec.	max.	
	fine		violet		violet		7500 - 10 000 RPM	10 000 RPM	
Refill Box of:	N Pressure:		Autoclavable:		Shank:		Medical device:		
6, 12, 25, 100	0,3 - 2N		135°C, 275°F		RA, stainless steel		Class IIa		





KENDA UNICUS

1-STEP DIAMOND POLISHING SYSTEM

- Polish porcelain and composites with the same polisher
- For an esthetic high luster result
- Ideal for anterior restorations
- No paste for high shine polishing needed
- Recommendation: Use fine grit finishing instruments or KENDA Nobilis before application




SET REF 0350.006A

10



REF reorder	0351	0352	0353	0355	0356	0358	0359	0360	0361
ISO 1: 838 204...	243 503 055	254 503 050	304 503 100	030 503 060	243 503 030	243 503 050	303 503 100	030 503 090	030 503 060
$\varnothing \times L$ mm	5,4 x 13	5 x 8	10 x 2	6,5 x 10	3 x 7	5 x 10	10 x 1	9 x 8,5	6 x 7,5
μ grit	extra-fine		color		orange		rec.	5000 - 7500 RPM	
μ max.	10.000 RPM		Refill Box of:		N Pressure:		Autoclavable:		Shank:
6, 12, 25, 100		0,3 - 2N		135°C, 275°F		RA, stainless steel		Medical device:	
								Class IIa	



KENDA COMPLETE

2-STEP POLISHING SYSTEM

- Multifunctional system balanced for a wide range of restorative materials
- Economic polishers with high performance abrasives
- Available in the most common shapes
- Higher gloss performance compared to other non-diamond systems



SET REF 0500.012A



REF	reorder	0505	0508	0509	0510	0555	0558	0559	0560
ISO	1 - 658 204 ... 2 - 658 204 ...	030 523 060	243 523 050	303 523 100	030 523 090	030 513 060	243 513 050	303 513 100	030 513 090
	∅ × L mm	6,5 x 10	5 x 10	10 x 1	9 x 8,5	6,5 x 10	5 x 10	10 x 1	9 x 8,5
	μ grit								
	color		light ruby colored			fine	steel-grey		
	rec.		7500 - 10 000 RPM		10 000 RPM		5000 - 7500 RPM		10 000 RPM
	max.								
	Refill Box of:	N Pressure:		Autoclavable:		Shank:		Medical device:	
	6, 12, 25, 100	0,3 - 2N		135°C, 275°F		RA, stainless steel		Class IIa	






KENDA MAXIMUS

1-STEP DIAMOND POLISHING SYSTEM

- Extremely efficient and time saving polishing on all composites
- From a scratched surface to an ultra luster in only one step
- High diamond content
- No paste for high shine polishing needed
- Optimized for Microhybrids and Nanofills



«This polisher has tested to give a significant better shine and finer surface.»

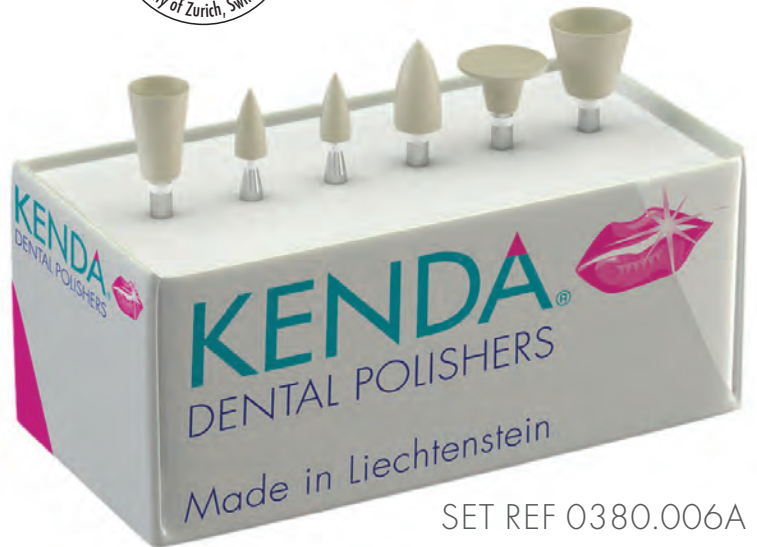


SET REF 0380.006A

12



REF reorder	0385	0386	0388	0389	0390	0391
ISO 1: 828 204	030 493 060	243 493 030	243 493 050	303 493 100	030 493 090	030 493 060
$\varnothing \times L$ mm	6.5 x 10	3 x 7	5 x 10	10 x 1	9 x 8.5	6 x 7.5
μ grit	ultra-fine		color		rec.	max.
	ultra-fine		light beige		5000 - 7500 RPM	10.000 RPM
Refill Box of:	N Pressure:		Autoclavable:	Shank:	Medical device:	
6, 12, 25, 100	0,3 - 2N		135°C, 275°F	RA, stainless steel	Class IIa	

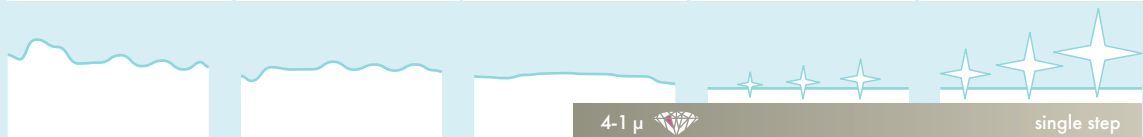



KENDA DELUXE

2-STEP DIAMOND POLISHING SYSTEM



- Deluxe double diamond combination for the most esthetic and high shine polish on all composite restorations
- Top choice for esthetic dentistry
- No additional paste for high shine polishing needed



SET REF 0400.006A



REF	reorder	0406	0408	0409	0411	0456	0458	0459	0461
ISO	1: 858 204 ... 2: 838 204 ...	243 513 030	243 513 050	303 513 100	030 513 060	243 503 030	243 503 050	303 503 100	030 503 060
	∅ × L mm	3 x 7	5 x 10	10 x 1	6 x 7,5	3 x 7	5 x 10	10 x 1	6 x 7,5
	μ grit								
	color								
	rec.								
	max.								
	μ grit								
	color								
	rec.								
	max.								
	Refill Box of:	N Pressure:		Autoclavable:		Shank:		Medical device:	
	6, 12, 25, 100	0,3 - 2N		135°C, 275°F		RA, stainless steel		Class IIa	






KENDA HYBRID

2-STEP POLISHING SYSTEM


- Optimized for hybrid composites and ceromer
- Firm and robust polisher facilitates exact adjustments
- Non-diamond prepolymer and diamond high shine polisher are the most economic combination to yield highly esthetic results
- Long lasting
- Gives ultra-smooth surfaces with high lustre

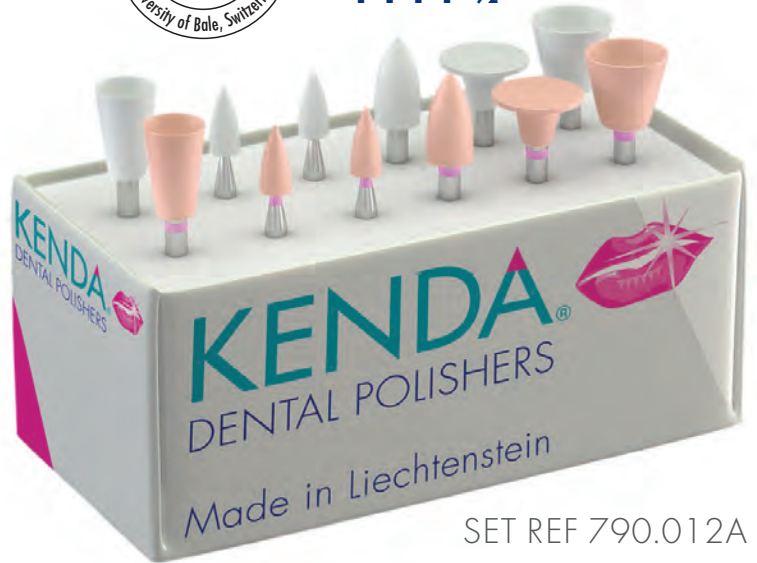

SET REF 790.012A



REF reorder	0005	0006	0008	0009	0010	0105	0106	0108	0109	0110
ISO 1: 632 204 ... 2: 822 204 ...	030 524 060	243 524 030	243 524 050	303 524 100	030 524 090	030 494 060	243 494 030	243 494 050	303 494 100	030 494 090
$\varnothing \times L$ mm	6,5 x 10	3 x 7	5 x 10	10 x 1	9 x 8,5	6,5 x 10	3 x 7	5 x 10	10 x 1	9 x 8,5
μ grit	color		rec.	max.	μ grit	color		rec.	max.	
medium	whitish grey		7500 - 10 000 RPM	10 000 RPM	ultra fine	pale pink		5000 - 7500 RPM	10 000 RPM	
Refill Box of:	N Pressure:		Autoclavable:		Shank:		Medical device:			
6, 12, 25, 100	0,3 - 2N		135°C, 275°F		RA, stainless steel		Class IIa			



KENDA MICROFILL

2-STEP POLISHING SYSTEM

- Optimized for microfilled composites
- Well proven basic polishing system in 2 steps
- Yellow polishers are also ideal to remove cement remnants of orthodontic bands (brackets)
- Available in a great variety of shapes






SET REF 750.012A



15

REF	reorder	4001	4003	4005	4006	4008	4009	4010	4011	5001	5003	5005	5006	5008	5009	5010	5011
ISO	638 204	243 523 055	304 523 100	030 523 060	243 523 030	243 523 050	303 523 100	030 523 090	030 523 060	243 493 055	304 493 100	030 493 060	243 493 030	243 493 050	303 493 100	030 493 090	030 493 060
	∅ × L mm	5,4x13	10x2	6,5x10	3x7	5x10	10x1	9x8,5	6x7,5	5,4x13	10x2	6,5x10	3x7	5x10	10x1	9x8,5	6x7,5
	μ grit	medium		yellow		7500 - 10 000 RPM		10 000 RPM		ultra fine		blue		5000 - 7 500 RPM		10 000 RPM	
	Rec. Box of:	N Pressure:		Autoclavable:		Shank:		Medical device:									
	6, 12, 25, 100	0,3 - 2N		135°C, 275°F		RA, stainless steel		Class IIa									

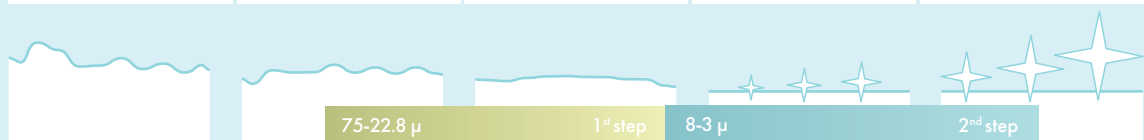

KENDA C.G.I.

3-STEP POLISHING SYSTEM

- Comprehensive polishing system with three grits
- Covering the whole process from contouring to high shine finish
- Flexible, adapting to tooth shape
- White polisher produces extra cutting efficacy for quick removal of excess material



SET REF 900.ASS.012



REF	reorder	905-C	908-C	909-C	910-C	905-M	908-M	909-M	910-M	905-F	908-F	909-F	910-F		
ISO	1: 638 204 2: 638 204... 3: 638 204...	030 533 060	243 533 050	303 533 100	030 533 090	030 523 060	243 523 050	303 523 100	030 523 090	030 493 060	243 493 050	303 493 100	030 493 090		
	∅ × L, mm	6,5 x 10	5 x 10	10 x 1	9 x 8,5	6,5 x 10	5 x 10	10 x 1	9 x 8,5	6,5 x 10	5 x 10	10 x 1	9 x 8,5		
	μ	grit	color	rec.	max.	μ	grit	color	rec.	max.	μ	grit	color	rec.	max.
		coarse	whitish white	7500 - 10 000 RPM	10 000 RPM	medium	green	3000 - 7500 RPM	10 000 RPM	ultra fine	pink	3000 - 7500 RPM	10 000 RPM		
	Refill Box of:	N Pressure:		Autoclavable:		Shank:		Medical device:							
	6, 12, 25, 100	0,3 - 2N		135°C, 275°F		RA, stainless steel		Class IIa							





KENDA ZIRCO1

1-STEP DIAMOND POLISHING SYSTEM

- From a scratched surface to an ultra luster in only one step
- For smoothing intraoral adjustments on all ceramic restorations including Zirconia and Lithium Disilicate
- Prevents abrasion of natural opposing teeth
- Reduces the risk of fracture and chipping
- No additional polishing paste required



SET REF 0230.006



REF reorder	0233	0240			
ISO ISO 204	243 514 060	030 514 090			
$\varnothing \times L$ mm	6 x 10.7	9 x 8.5			
μ grit	color	rec.	max.		
fine	green	7500 - 15 000 RPM	15 000 RPM		
Refill Box of:	N Pressure:	Autoclavable:	Shank:	Medical device:	
6, 12, 25, 100	0,3 - 2N	135°C, 275°F	RA, stainless steel	Class IIa	





KENDA ZIRCOVIS

2-STEP DIAMOND POLISHING SYSTEM

- Firm and robust polisher
- For smoothing intraoral adjustments on all ceramic restorations including Zirconia and Lithium Disilicate
- Prevents abrasion of natural
- opposing teeth
- Reduces the risk of fracture and chipping
- Long lasting
- No additional polishing paste required



SET REF 0250.006A

18



REF	reorder	0255	0256	0258	0265	0266	0268	
ISO	1 - B62 204 ... 2 - B52 204 ...	030 524 060	243 524 030	243 524 050	030 514 060	243 514 030	243 514 050	
	∅ × L mm	6,5 x 10	3 x 7	5 x 10	6,5 x 10	3 x 7	5 x 10	
	μ grit	color	rec.	max.	μ grit	color	rec.	max.
	medium	dark blue-green	7500 - 10 000 RPM	10 000 RPM	fine	light blue-green	5000 - 7 500 RPM	10 000 RPM
	Refill Box of:	N Pressure:	Autoclavable:	Shank:	Medical device:			
	6, 12, 25, 100	0,3 - 2N	135°C, 275°F	RA, stainless steel	Class IIa			





KENDA ALL CERAMIC

2-STEP DIAMOND POLISHING SYSTEM


- Flexible polisher for all ceramic restorations
- Adapts to tooth shape
- Prevents abrasion of natural opposing teeth
- Reduces the risk of fracture and chipping



SET REF 0200.006A



REF	reorder	0215	0216	0218	0219	0225	0226	0228	0229
ISO	1 : 868 204 ... 2 : 838 204 ...	030 523 060	243 523 030	243 523 050	303 523 100	030 503 060	243 503 030	243 503 050	303 503 100
	∅ × L mm	6,5 x 10	3 x 7	5 x 10	10 x 1	6,5 x 10	3 x 7	5 x 10	10 x 1
	μ grit								
	color		medium bordeaux			extra-fine	light bordeaux		
	rec.			7500 - 10 000 RPM				5000 - 7 500 RPM	
	max.			10 000 RPM				10 000 RPM	
	Refill Box of:	N Pressure:		Autoclavable:		Shank:		Medical device:	
	6, 12, 25, 100	0,3 - 2N		135°C, 275°F		RA, stainless steel		Class IIa	



KENDA PROPHY

1-STEP POLISHING SYSTEM

- For Tooth Cleaning on Natural Enamel
- Gently removes extrinsic stains without polishing paste
- Fine abrasive grit is already interspersed in the head
- Is firmer than common prophycups which allows easy control for specific removal
- Ideal for small esthetic corrections





SET REF 5100.012

20



REF reorder	5105	5106	5108	5110
ISO 1: 658 204...	030 523 060	243 523 030	243 523 050	030 523 090
$\varnothing \times L$ mm	6,5 x 10	3 x 7	5 x 10	9 x 8,5
μ grit	medium		color	blue
rec.	7500 - 10 000 RPM		max.	10 000 RPM
Refill Box of:	N Pressure:	Autoclavable:	Shank:	Medical device:
6, 12, 25, 100	0,3 - 2N	135°C, 275°F	RA, stainless steel	Class IIa

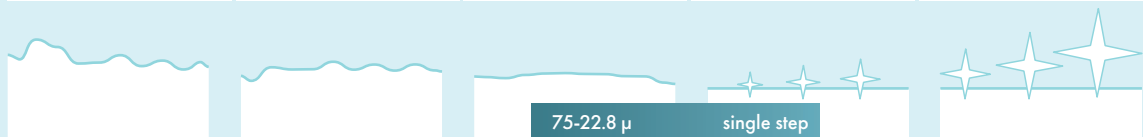

KENDA PLANUS

2-STEP SMOOTHING AND POLISHING SYSTEM



- Polisher for intra-oral use on acrylics
- Autoclavable
- Ideal for chairside adjustments on mouthguards, retainers, acrylic dentures and even snoring mouth pieces



SET REF 0600.012




REF reorder	0601	0608			0611	0618		
ISO 1: 638 204 ... 2: 638 204 ...	243 533 055	243 533 050			243 513 055	243 513 050		
21 31 ∅ x L mm	5,4 x 13	5 x 10			5,4 x 13	5 x 10		
μ grit	color	rec.	max.	μ grit	color	rec.	max.	
coarse	lime-green	7500 - 10 000 RPM	10 000 RPM	fine	grey	5000 - 7500 RPM	10 000 RPM	
Refill Box of:	N Pressure:	Autoclavable:	Shank:		Medical device:			
6, 12, 25, 100	0,3 - 2N	135°C, 275°F	RA, stainless steel		Class IIa			

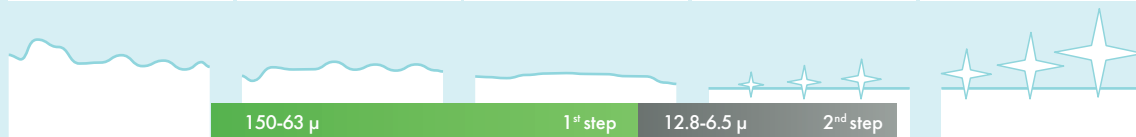

KENDA AMALGAM

2-STEP POLISHING SYSTEM



- Optimized for amalgam restorations
- Time tested system
- Impregnated with high quality abrasives
- Available in a wide array of shapes

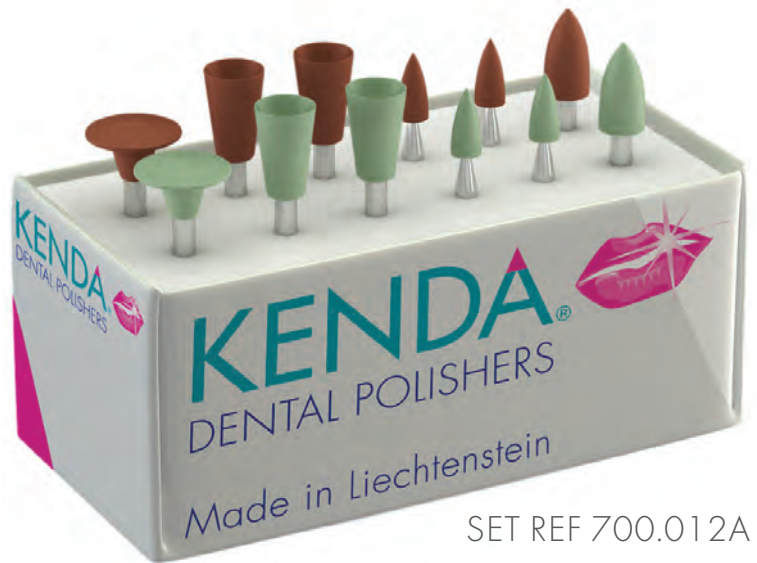

SET REF 700.012A



REF	reorder	2001	2003	2005	2006	2008	3001	3003	3005	3006	3008
ISO	1 - 658 204 ... 2 - 658 204 ...	243 523 055	304 523 100	030 523 060	243 523 030	243 523 050	243 513 055	304 513 100	030 513 060	243 513 030	243 513 050
	∅ × L mm	5,4 x 13	10 x 2	6,5 x 10	3 x 7	5 x 10	5,4 x 13	10 x 2	6,5 x 10	3 x 7	5 x 10
	μ grit										
	color										
	rec.										
	max.										
	μ grit										
	color										
	rec.										
	max.										
	Refill Box of:	N Pressure:		Autoclavable:		Shank:		Medical device:			
	6, 12, 25, 100	0,3 - 2N		135°C, 275°F		RA, stainless steel		Class IIa			

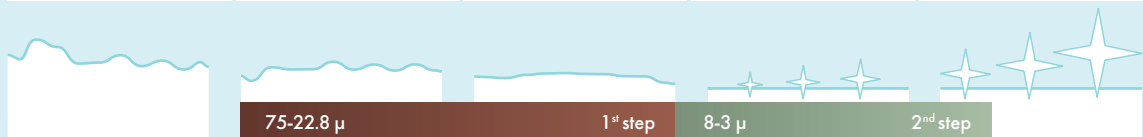




KENDA PRECIOUS METALS

2-STEP POLISHING SYSTEM



- The most esthetic solution for all metals
- Cost saving combination of non-diamond prepolisher and diamond high-shine polisher
- Mirror luster results

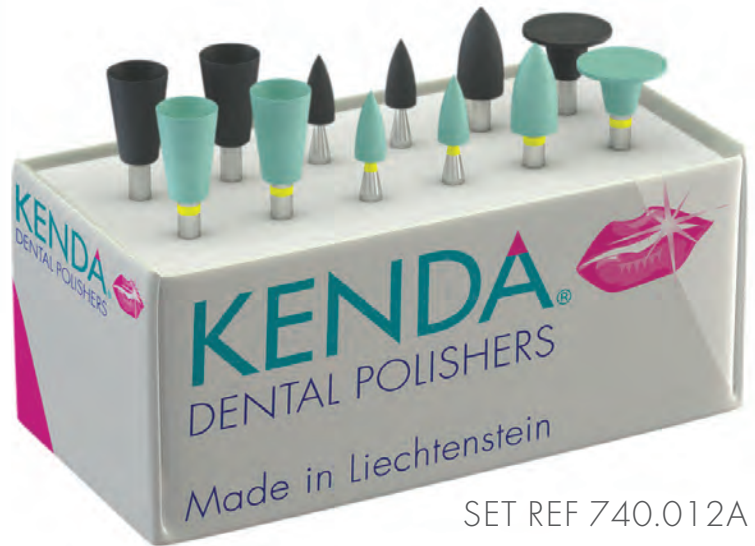

SET REF 740.012A



REF	reorder	1005	1006	1008	1009	1105	1106	1108	1109
ISO	1 - 652 204 ... 2 - 832 204 ...	030 524 060	243 524 030	243 524 050	303 524 100	030 504 060	243 504 030	243 504 050	303 504 100
	∅ x L mm	6,5 x 10	3 x 7	5 x 10	10 x 1	6,5 x 10	3 x 7	5 x 10	10 x 1
	μ grit								
	color		black			extra-fine	green		
	rec.			7500 - 10 000 RPM				5000 - 7 500 RPM	
	max.			10 000 RPM				10 000 RPM	
	Refill Box of:	N Pressure:		Autoclavable:		Shank:		Medical device:	
	6, 12, 25, 100	0,3 - 2N		135°C, 275°F		RA, stainless steel		Class IIa	

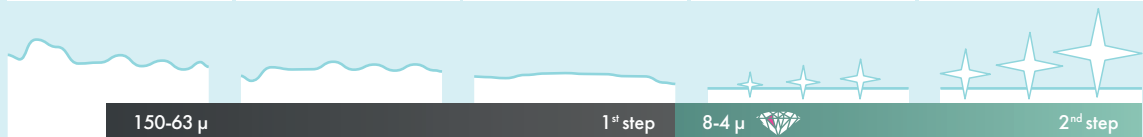


CLINICAL SINGLE-USE



CLINICAL

SINGLE-USE POLISHERS




Polishers for the intra-oral use on a single patient.

Reduces the risk of cross-contamination.



Single-use polishers always make the polishing procedure begin with a perfectly shaped polisher for preciser polishing.



No time-consuming cleaning and reprocessing.



Polishette

mini shaped polishers


- Mini shaped polishers with tapered shank necks
- Superior precision
- More space to work, better access, increased visibility
- Three grits cover all tasks from contouring to high shine finish
- Single-use for convenience



SET REF PS710X.024



REF	reorder	PS715C	PS716C	PS715M	PS716M	PS715F	PS716F							
ISO	1 - 650 244 2 - 630 244 3 - 830 244	030 543 060	243 543 030	030 523 060	243 523 030	030 503 060	243 503 030							
	∅ × L, mm	6,5 x 5	3 x 7	6,5 x 5	3 x 7	6,5 x 5	3 x 7							
μ	grit	color	rec.	max.	μ	grit	color	rec.	max.	μ	grit	color	rec.	max.
	coarse	green	5 000 RPM	5 000 RPM	medium	red	5 000 RPM	5 000 RPM		extra-fine	purple	5 000 RPM	5 000 RPM	
	Refill Box of:	N Pressure:		Single-Use		Shank:		Medical device:						
	15 (diamond), 30 (non-diamond)	0.3-1N		disposable		RA, medical plastic		Class IIa						





DISPOSABLE KENDA G.P.S

2-STEP DIAMOND POLISHING SYSTEM

- Double diamond combination for the most esthetic polish and high shine on all composite restorations
- Top choice for esthetic dentistry
- No additional paste for high shine polishing needed



SET REF PS0400.012




REF reorder	PS0409	PS0411	PS0412	PS0459	PS0461	PS0462	
ISO 1: 858 242... 2: 838 242...	303 513 100	030 513 060	243 513 045	303 503 100	030 503 060	243 503 045	
$\varnothing \times L$ mm	10 x 1	6 x 7,5	5 x 10	10 x 1	6 x 7,5	5 x 10	
μ grit	color	rec.	max.	μ grit	color	rec.	max.
fine	light green	5000 RPM	5000 RPM	extra-fine	light-beige	5000 RPM	5000 RPM
Refill Box of:	N Pressure:		Single-Use	Shank:		Medical device:	
6, 12, 25, 100	0,3 - 1N		disposable	RA, medical plastic		Class IIa	



DISPOSABLE KENDA BIG JOB

1-STEP POLISHING SYSTEM


- Fast and easy finishing and polishing
- Ideal for quick adjustments and smoothing large restoration surfaces
- Recommendation: For ultimate high shine use KENDA G.P.S. diamond high shine polisher

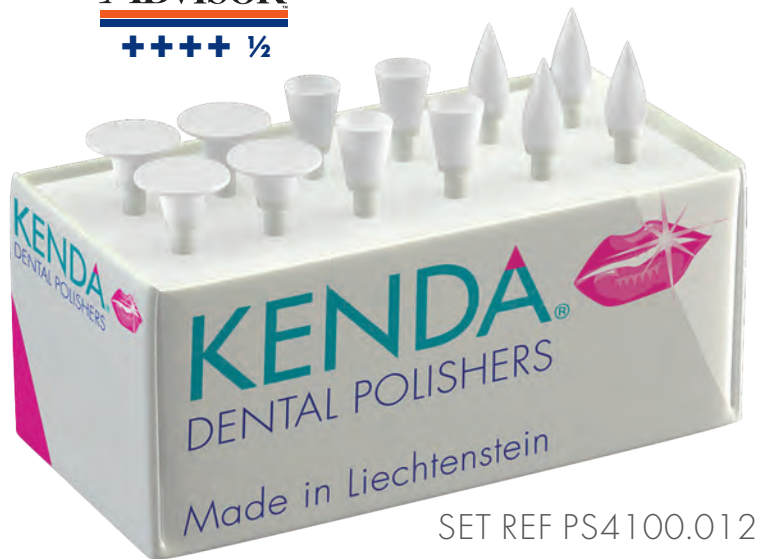


SET REF PS4100.012



REF reorder	PS4109	PS4111	PS4112
ISO 1 : 638 242 ...	303 523 100	030 523 060	243 523 045
Ø × L mm	10 × 1	6 × 7,5	5 × 10
μ grit	medium	color	white
rec.	5000 RPM	max.	5000 RPM
Refill Box of:	6, 12, 25, 100	N Pressure:	0,3 - 1N
		Single-Use:	disposable
		Shank:	RA, medical plastic
		Medical device:	Class IIa




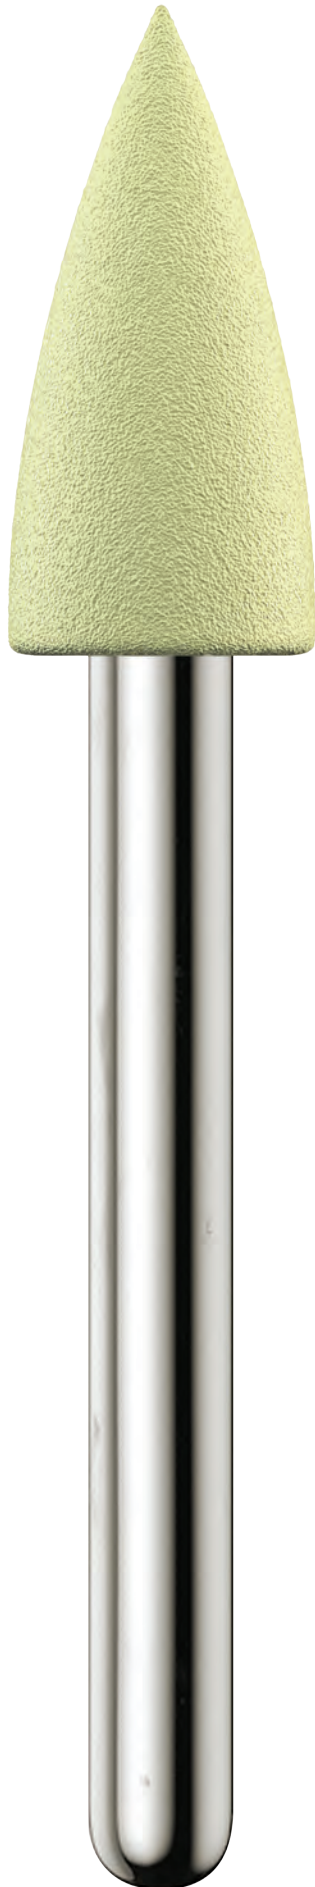

CLINICAL

FG POLISHERS

Polishers on friction grip shanks for high speed handpieces. FG-polishers facilitate the restoration procedure - No changing of the handpiece is necessary after using FG-finishing instruments.



Can be autoclaved and used on multiple patients



Use with maximum speed of 20'000 rpm
Do not use with air turbine

FG

KENDA FG SERIES



2 step diamond polishing system for all composites and porcelain. For very efficient polishing.


REF reorder	0306FG	0386FG					
ISO 1 - 822 313 ... 2 - 822 313 ...	243 514 030	243 494 030					
$\varnothing \times L$ mm	3 x 7	3 x 7					
grit	color	rec.	max.	grit	color	rec.	max.
fine	violet	20 000 RPM	20 000 RPM	ultra-fine	light biege	10 000 RPM	20 000 RPM
Refill Box of:	N Pressure:	Autoclavable:	Shank:		Medical device:		
6	0,3 - 2N	135°C, 275°F	FG, stainless steel		Class IIa		



2-step polishing system for all composites


29

REF reorder	4006FG	5006FG					
ISO 1 - 632 313 ... 2 - 632 313 ...	243 524 030	243 494 030					
$\varnothing \times L$ mm	3 x 7	3 x 7					
grit	color	rec.	max.	grit	color	rec.	max.
medium	yellow	20 000 RPM	20 000 RPM	ultra-fine	blue	10 000 RPM	20 000 RPM
Refill Box of:	N Pressure:	Autoclavable:	Shank:		Medical device:		
6	0,3 - 2N	135°C, 275°F	FG, stainless steel		Class IIa		

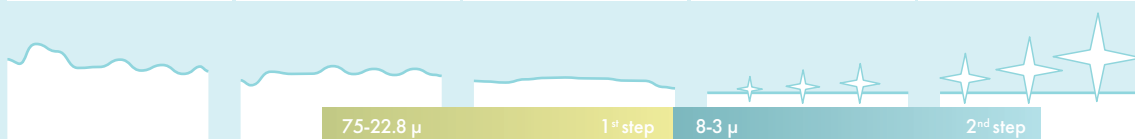

2-step polishing system for amalgam and precious metals.

REF reorder	2006FG	3006FG					
ISO 1 - 652 313 ... 2 - 652 313 ...	243 524 030	243 514 030					
$\varnothing \times L$ mm	3 x 7	3 x 7					
grit	color	rec.	max.	grit	color	rec.	max.
medium	brown	20 000 RPM	20 000 RPM	fine	green	10 000 RPM	20 000 RPM
Refill Box of:	N Pressure:	Autoclavable:	Shank:		Medical device:		
6	0,3 - 2N	135°C, 275°F	FG, stainless steel		Class IIa		

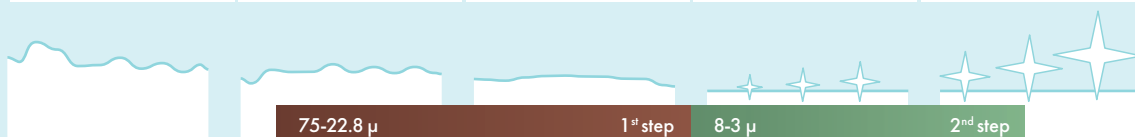

LABORATORY



LABORATORY

POLISHERS

Polishers in big shapes for extra-oral application on large surfaces. Feature long shanks for laboratory handpieces. The KENDA Laboratory Line offers high-end solutions for Ceramics, Acrylic Dentures and other materials.





KENDA Z-SERIES

3-STEPS DIAMOND POLISHING SYSTEM

- For all types of ceramics including Zirconia, Alumina and Lithium Disilicate
- High diamond content for superior efficiency
- Three different grits cover all tasks from adjustment to high shine polishing
- Fast adjustments with the coarse purple polisher
- Smooth result minimizes abrasion of opposing natural teeth
- Reduces chipping and breakage



SET REF Z-000.009



31

REF	reorder	Z-006-C	Z-010-C	Z-014-C	Z-006-M	Z-010-M	Z-014-M	Z-006-F	Z-010-F	Z-014-F		
ISO	1 - 872 104 2 - 862 104... 3 - 852 104...	243 534 030	041 534 120	041 534 120	243 524 030	041 524 120	041 524 120	243 514 030	041 514 120	041 514 120		
	∅ × L mm	3 x 7	12 x 2,5	12 x 2	3 x 7	12 x 2,5	12 x 2	3 x 7	12 x 2,5	12 x 2		
	μ grit	coarse			medium			fine				
	color	violet			petrol			lime				
	rec.	7500 - 10 000 RPM			7500 - 10 000 RPM			5000 - 7500 RPM				
	max.	10 000 RPM			10 000 RPM			10 000 RPM				
	Refill Box of:	3			Pressure:	0,3 - 2N			Shank:	HP, stainless steel		





KENDA HIGH END

4-STEP DIAMOND POLISHING SYSTEM

- For all types of ceramics including Zirconia, Alumina and Lithium Disilicate
- The best solution for ultimate results
- Extra high diamond content
- Finely balanced in 4 grits
- High peripheral speed
- Designed for optimal interdental work
- Prevents abrasion of opposing natural teeth
- Reduces chipping and breakage



SET REF 626.004


32



REF reorder	626-C	626-M	626-F	626-XF
ISO	872 104 303 534 260	862 104 303 524 260	852 104 303 514 260	832 104 303 504 260
$\varnothing \times L$ mm	26 x 2	26 x 2	26 x 2	26 x 2
grit	coarse	medium	fine	extra-fine
color	violet	pink	green	grey
rec.	7 500 - 10 000 RPM	7 500 - 10 000 RPM	7 500 - 10 000 RPM	5 000 - 7 500 RPM
max.	10 000 RPM	10 000 RPM	10 000 RPM	10 000 RPM
Box of:	1			
Pressure:		0,3 - 2N		
Shank:				HP, stainless steel




KENDA WHEEL & KNIFE

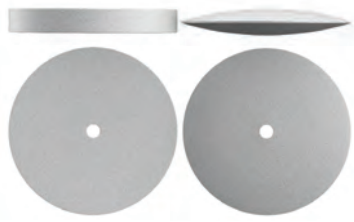

- Fast results on large surfaces
- High edge stability
- Cost effective solution


Ceramic prepolisher for fast smoothing of all silicate ceramics.

REF reorder	6522-R	6522-L		
ISO 1: 658 900 ...	372 533 220	303 533 220		
$\varnothing \times L$ mm	22 x 3	22 x 3		
grit	coarse		color	light grey
			rec.	20 000 RPM
			max.	20 000 RPM

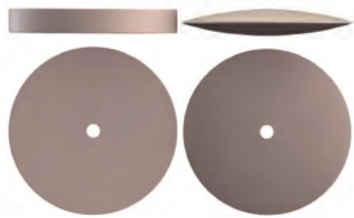


Ceramic high shine polisher for final shine.

REF reorder	7522-R	7522-L		
ISO 1: 658 900 ...	372 513 220	303 513 220		
$\varnothing \times L$ mm	22 x 3	22 x 3		
grit	fine		color	pale pink
			rec.	10 000 RPM
			max.	20 000 RPM

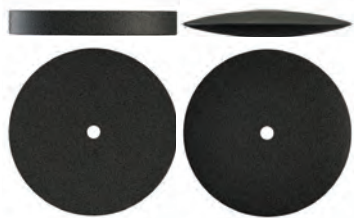

Universal polisher, for polishing all alloys and acrylic dentures.

REF reorder	1522-R	1522-L		
ISO 1: 658 900 ...	372 523 220	303 523 220		
$\varnothing \times L$ mm	22 x 3	22 x 3		
grit	medium		color	black
			rec.	20 000 RPM
			max.	20 000 RPM
Refill Box of:	10, 100		Pressure:	0,3 - 2N
			Shank:	unmounted

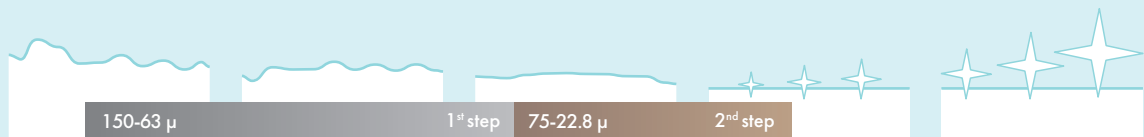

KENDA RED

1-STEP POLISHING SYSTEM

- Optimized for use on acrylics combined with chrome cobalt alloys
- Polishes the acrylic without damaging the alloy
- Single grit, ideal for finishing and polishing



REF RED 14.006

34



REF reorder	RED 8	RED 14		
ISO 1: 658 104...	245 523 125	204 523 100		
$\varnothing \times L$ mm	12,5 x 22	10 x 24,5		
μ grit	medium	red	rec.	max.
			10 000 - 15 000 RPM	15 000 RPM
Box of:	N Pressure:		Shank:	
6, 12, 25, 100	0,3 - 2N		HP, stainless steel	



KENDA QUEEN

2-STEP FINISHING AND POLISHING SYSTEM

- Long lasting, time tested system
- Two balanced grits available
- Firm sharp abrasive grit for a faster polishing finish




REF reorder	9008	9009	9010	9013	9014	9015	9016
ISO 1-658 104...	245 533 125	144 533 125	237 533 120	114 533 085	204 533 100	243 533 100	213 533 065
Ø x L mm	12,5 x 22	12,5 x 15	12 x 17	8,5 x 18	10 x 24,5	10 x 18	6,5 x 17
grit	coarse		color		rec.		max.
			green		10 000 - 15 000 RPM		15 000 RPM



35

REF reorder	7008	7009	7010	7013	7014	7015	7016
ISO 1-658 104...	245 523 125	144 523 125	237 523 120	114 523 085	204 523 100	243 523 100	213 523 065
Ø x L mm	12,5 x 22	12,5 x 15	12 x 17	8,5 x 18	10 x 24,5	10 x 18	6,5 x 17
grit	medium		color		rec.		max.
			black		10 000 - 15 000 RPM		15 000 RPM
Box of:			N Pressure:		Shank:		
	6, 12, 25, 100		0,3 - 2N		HP, stainless steel		

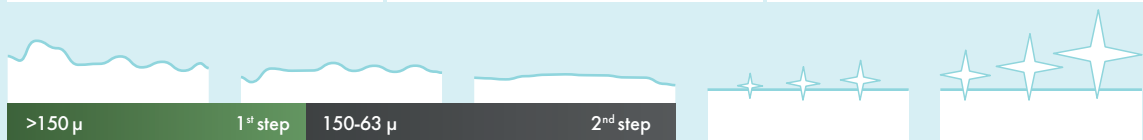

KENDA ACRYLIC BLUE

3-STEPS POLISHING SYSTEM




REF reorder	8308	8314	8315	8408	8414	8415	
ISO 1 - 630 104 ... 2 - 630 104 ...	245 543 125	204 543 100	243 543 100	245 523 125	204 523 100	243 523 100	
$\varnothing \times L$ mm	12,5 x 22	10 x 24,5	10 x 18	12,5 x 22	10 x 24,5	10 x 18	
μ grit	color	rec.	max.	μ grit	color	rec.	max.
very coarse	blue	10 000 - 15 000 RPM	15 000 RPM	medium	light blue	10 000 - 15 000 RPM	15 000 RPM

36



- Long lasting, time tested system
- Three balanced grits available
- Soft sharp abrasive grit - for a smooth polishing feel
- Coarse grit allows for easy and quick adjustments

REF reorder	8508	8514	8515
ISO 1 - 630 104 ...	245 503 125	204 503 100	243 503 100
$\varnothing \times L$ mm	12,5 x 22	10 x 24,5	10 x 18
μ grit	color	rec.	max.
extra-fine	ochre	5000-10000 RPM	15 000 RPM
Refill Box of:	N Pressure:		Shank:
6, 12, 25, 100	0,3 - 2N		HP, stainless steel

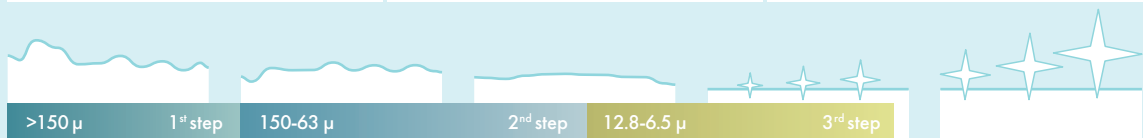

KENDA YELLOW LINE

- Fine polisher ideal for the dental practice to make small adjustments
- Fine grit prevents over-adjustments
- Spiral Wheel for easy polishing of interdental areas



SET REF Y-000.003A



37

REF reorder	Y-008	Y-014	Y-019
ISO 1: 638 104...	056 523 150	204 523 100	543 523 190
$\varnothing \times L$ mm	12,5 x 22	10 x 24,5	19 x 0,5
μ grit	medium	yellow	7 500 - 10 000 RPM
color	yellow	7 500 - 10 000 RPM	10 000 RPM
rec.	7 500 - 10 000 RPM	10 000 RPM	
max.	10 000 RPM		
Refill Box of:	N Pressure:		Shank:
3	0,3 - 2N		HP, stainless steel



KENDA PLANUS


2-STEP SMOOTHING AND POLISHING SYSTEM

- Autoclavable polisher in lab shapes made of high quality medical silicone
- Designed for smoothing pressure spots
- Ideal for acrylic dentures, as well as retainers, mouthguards, and even snoring mouth pieces




SET REF 6700.006

38

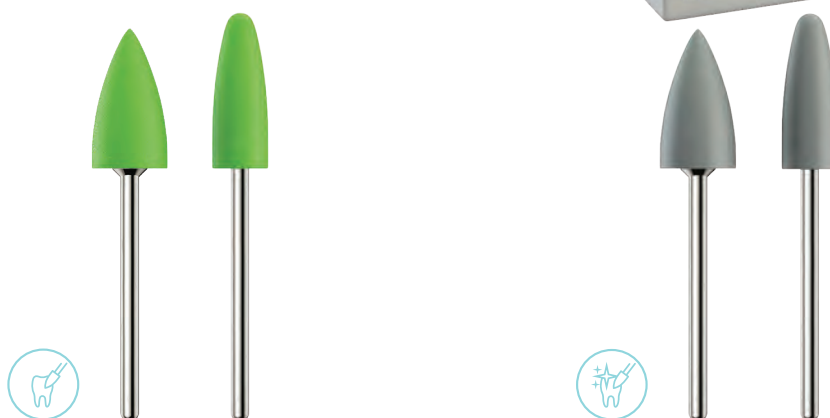

REF	reorder	6715	6720	6815	6820				
ISO	1: 638 104...	243 533 100	497 533 070	243 513 100	497 513 070				
	∅ × L mm	10 x 18	7.2 x 20	10 x 18	7.2 x 20				
μ	grit	color	rec.	max.	μ	grit	color	rec.	max.
	coarse	lime-green	10 000 - 15 000 RPM	15 000 RPM		fine	grey	10 000 - 15 000 RPM	15 000 RPM
Refill Box of:			N Pressure:		Shank:				
6, 12, 25, 100			0,3 - 2N		HP, stainless steel				

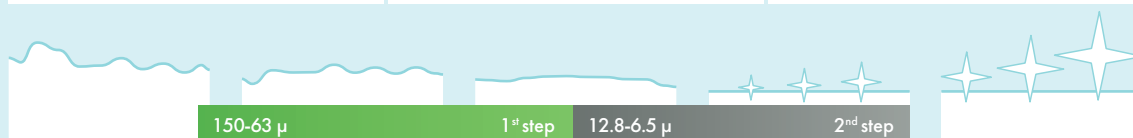

KENDA BESTFLEX

1-STEP POLISHING SYSTEM

- Specially adapted to nylon based flexible dentures
- Just one step for a smooth finish, available in three shapes



SET REF 6500.006



REF reorder	6508	6514	6516	
ISO 1: 658 104...	245 533 125	204 533 100	213 533 065	
2 3 $\varnothing \times L, mm$	12,5 x 22	10 x 24,5	6,5 x 17	
μ grit	color		rec.	max.
coarse	white grey		10 000 - 15 000 RPM	15 000 RPM
Refill Box of:	N Pressure:		Shank:	
6, 12, 25, 100	0,3 - 2N		HP, stainless steel	





KENDA PRECIOUS METALS


2-STEP POLISHING SYSTEM

- The preferred system for titanium alloys, precious & non precious metals
- Highly esthetic finish
- Cost effective combination of non-diamond prepolisher and diamond high shine polisher
- Mirror luster results




SET REF 741.006


40

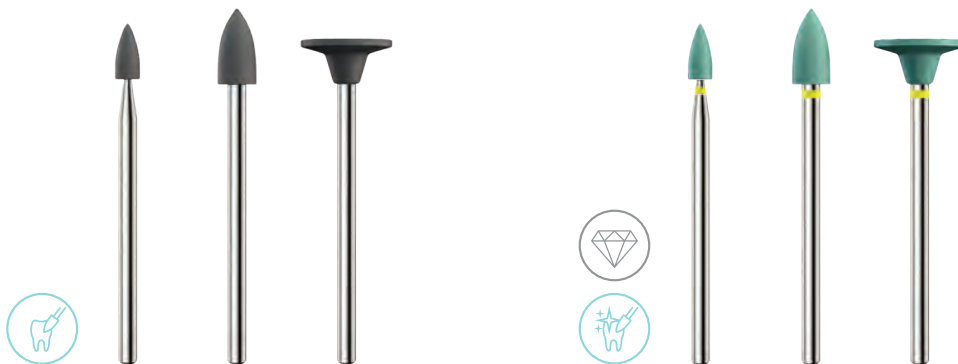

REF reorder	1006HP	1008HP	1014HP	1106HP	1108HP	1114HP	
ISO 1: 652 104 ... 2: 832 104 ...	243 524 030	243 524 050	041 524 120	243 504 030	243 504 050	041 504 120	
21 31 ∅ × L mm	3 x 7	5 x 10	12 x 2	3 x 7	5 x 10	12 x 2	
grit	color	rec.	max.	grit	color	rec.	max.
medium	black	7 500 - 10 000 RPM	10 000 RPM	extra-fine	green	5 000 - 7 500 RPM	10 000 RPM
Refill Box of:			N Pressure:			Shank:	
6, 12, 25, 100			0,3 - 2N			HP, stainless steel	

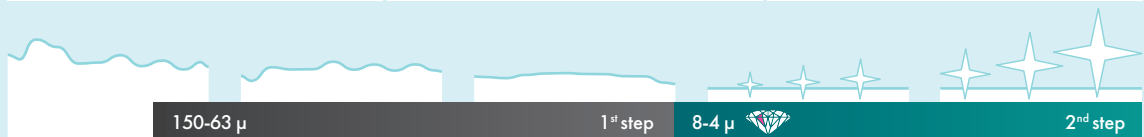


KENDA WHEEL & KNIFE

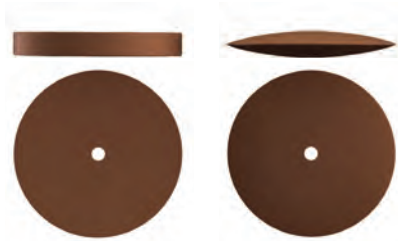

- Fast results on large surfaces
- High edge stability
- Cost effective solution

Gold prepolisher, for gold and semi precious alloys.

REF reorder	2522R	2522-L		
ISO 1: 658 900...	372 513 220	303 513 220		
$\varnothing \times L$ mm	22 x 3	22 x 3		
grit	fine		color	brown
			rec.	20 000 RPM
			max.	20 000 RPM

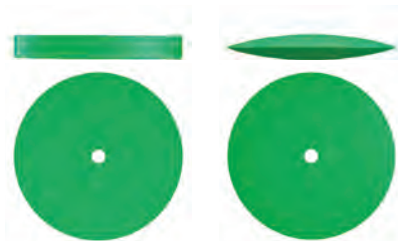


Gold high shine polisher, for high shine on gold and semi-precious alloys.

REF reorder	3522-R	3522-L		
ISO 1: 658 900...	372 503 220	303 503 220		
$\varnothing \times L$ mm	22 x 3	22 x 3		
grit	extra fine		color	green
			rec.	10 000 RPM
			max.	20 000 RPM



Titanium polisher, eliminates scratches and smoothes all titanium surfaces

REF reorder	9522-R	9522-L		
ISO 1: 658 900...	372 533 220	303 533 220		
$\varnothing \times L$ mm	22 x 3	22 x 3		
grit	coarse		color	oliv
			rec.	20 000 RPM
			max.	20 000 RPM
Refill Box of:	10, 100		N Pressure:	0,3 - 2N
			Shank:	unmounted

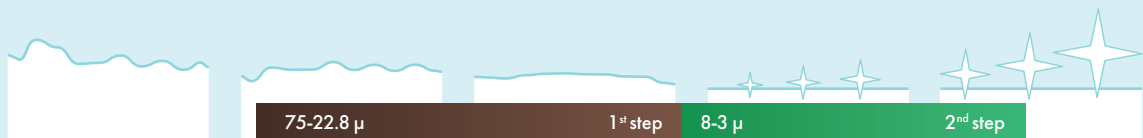



KENDA HYBRID

2-STEP POLISHING SYSTEM

- The solution for indirect composite restorations
- Non-diamond prepolymer and diamond high shine polisher are the most cost effective solution to yield highly esthetic results
- Firm and robust



SET REF 791.006

42



REF reorder	0006HP	0008HP	0014HP	0106HP	0108HP	0114HP	
ISO 1 : 632 104 ... 1 : 822 104 ...	243 524 030	243 524 050	041 524 120	243 494 030	243 494 050	041 494 120	
$\varnothing \times L$ mm	3 x 7	5 x 10	12 x 2	3 x 7	5 x 10	12 x 2	
μ grit	color	\circlearrowright rec.	\circlearrowright max.	μ grit	color	\circlearrowright rec.	\circlearrowright max.
medium	whitish grey	7 500 - 10 000 RPM	10 000 RPM	ultra-fine	pale pink	5 000 - 7 500 RPM	10 000 RPM
Box of:	N Pressure:		Shank:				
6, 12, 25, 100	0,3 - 2N		HP, stainless steel				



KENDAPRACTICUS

- KENDA PRACTICUS offers space for 6 RA polishers of 22-31 mm length and 12 FG diamond instruments of 16 to 24 mm length.
- Thanks to well thought out alignment, ergonomic handling with only one hand is possible. Due to the snap lock the caddy can be easily closed and content is fixed for sterilization. The high-tech medical polymer allows up to 3000 sterilization cycles in the autoclave at 135 °C, 275 °F.



REF 270




REF 271



REF 272



REF 273

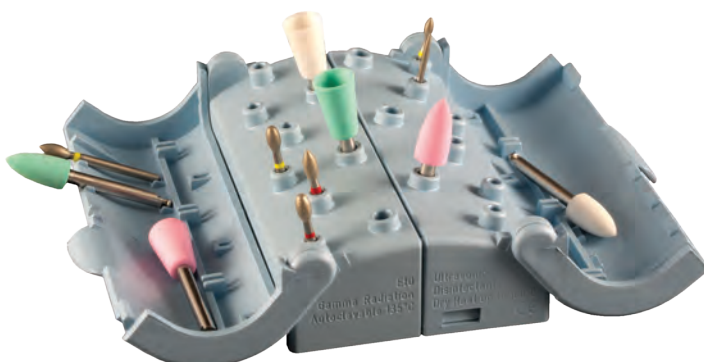



DIAMOND POLISHERS

Diamond polishers contain abrasive particles from natural or synthetic diamond. Due to their exceptional hardness (10 according to the Mohs Hardness Scale), they offer superior cutting efficiency which results in:



1. Less polishing time,



2. Lower surface roughness values



3. Superior gloss values (select a fine diamond polisher from our application range graphic which is suitable for high shine polishing to receive significantly better gloss values than with standard non-diamond polishers).



4. Longer durability



Look for the diamond logo on the product pages to see if a certain polisher is diamond impregnated.

KENDA PACKAGING

OUR POLISHERS ARE AVAILABLE IN STARTER-KITS AND REFILL BOXES

STARTER KITS

contain 6 or 12 polishers, comprise all grit sizes offered for a specific system and come with mixed shapes.

Example: The Starter-Kit of KENDA C.G.I.

- 4 white (coarse grit) polishers in different shapes
- 4 green (medium grit) polishers in different shapes
- 4 pink (fine grit) polishers in different shape



REFILL BOXES

contain a different amount of one specific shape in one specific grit.

- Refill box of 6 polishers



KENDA PACKAGING

- Refill box of 12 polishers



- Refill box of 25 polishers




46

- Refill box of 100 polishers



EXPLAINING THE LABEL

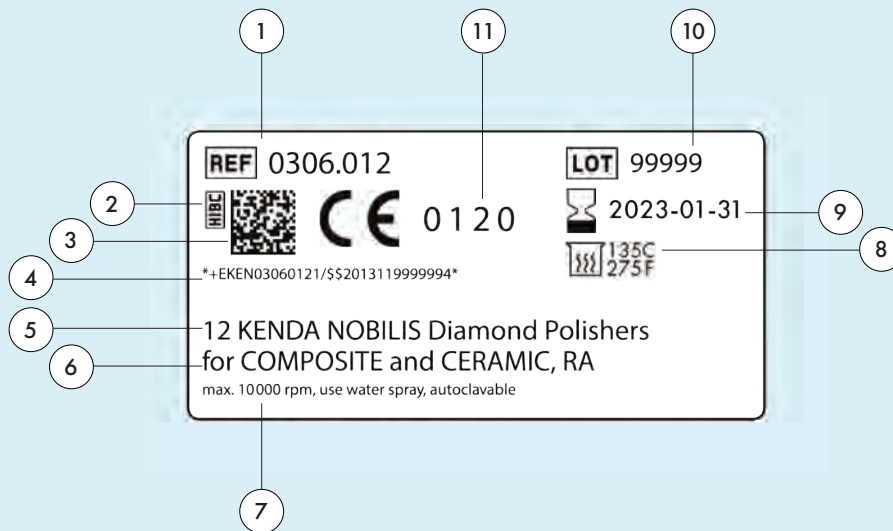

The label that you can find on all of our products is designed according to latest standards and has a lot of information on it. It is readable for humans as well as for barcode scanners. The barcode is in the format of «HIBC Data Matrix» which can hold a lot of information. In this example label, the barcode contains our unique HIBC labeler identification code (EKEN), REF, expiration date as well as the LOT number.

Labels can vary for certain products and countries.

1	order number
2	HIBC logo to identify barcode
3	machine readable barcode
4	human readable barcode information
5	quantity and product name
6	application
7	max. RPM, security advices
8	information for sterilization
9	expiration date (yyyy-mm-dd)
10	LOT number
11	CE mark with notified body

SIGNS AT A GLANCE

Pictographs will appear to indicate the specific use of the instrument.



Polisher for smoothing and finishing



Diamond particles as material of working part for efficient polishing



Polisher for finishing and silky shine polishing



Maximum speed in RPM. Do not exceed.



High shine polisher for ultimate gloss



Recommended speed in RPM for best polishing results.



Autoclavable with moist heat sterilization



Disposable. Use one time only.



Use waterspray for cooling



Packaging units in boxes



Order number



CE-sign confirms conformity with Directive 93/42/EEC



LOT number – for traceability of the respective production batch



Color



Expiry date



Storage temperature



Manufacturer



Keep away from sunlight



User instructions / refer to catalogue



Wear breathing protection



Wear eye protection

WHY POLISH?

HEALTH

Polishing eliminates rough surfaces which would otherwise produce plaque accumulation and run the risk of secondary-recurrent caries. Polishing thus makes restorations longer lasting. Unpolished surfaces near the gingiva can also increase the risk of periodontitis.

COMFORT

The human tongue is able to detect differences in roughness in a range as low as a micrometer. Therefore, a polished filling will create a pleasant feeling for the patient.

ESTHETICS

Polishing helps to achieve an esthetic finish by reducing surface staining and producing a natural shine finish.

THE CONSTRUCTION OF A DENTAL POLISHER

POLISHING HEAD

1

The polishing head is made up of either silicone or synthetic rubber, mixed in with abrasive particles made of diamond, silicon carbide or aluminum oxide. The various mixtures provide the required polishing effects. Some polishers are not active themselves and require the additional use of a polishing paste (in particular for prophylaxis).

All KENDA Polishers contain abrasive particles and do not need to be used with polishing paste.

SHANK

2


Shanks for polishers come in either stainless steel or plastic for multi-use or single-use respectively.

Shanks also come in different types:


FG friction grip Ø 1,6 mm



RA contra angle Ø 2,35 mm



HP hand piece Ø 2,35 mm

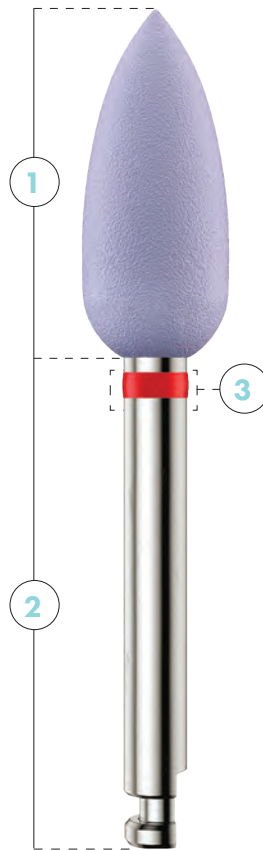

COLORED RING

3

The colored rings on the shank indicate the different diamond grit sizes according to ISO 21671.


Color grit size in micron

□	ultra-fine	4 - 1 μ
■	extra-fine	8 - 4 μ
■	fine	32 - 8 μ
■	medium	69 - 32 μ
■	coarse	164 - 69 μ
■	very coarse	>164 μ

POLISHER SHAPES & USAGE



POINTS

Points are ideal for polishing both the cervical area and the occlusal grooves and reliefs. For some systems, up to four different points and sizes are available to satisfy dentists' individual preferences.




CUPS

There are three different cup sizes. They can be used in different application areas, such as on cusp slopes of posterior teeth, proximal line angle areas and on buccal, lingual, and palatal surfaces of anterior restorations.



DISCS

There are two different types of discs. Both are ideal on incisors, large filling surfaces, incisal edges and inter-proximal areas.



POLISHING SYSTEMS




1-STEP POLISHING SYSTEM

This system contains only one single polisher which usually has diamond particles as an abrasive. It achieves good polishing results solely by altered pressure application by the dentist. The user pre-polishes with more pressure and achieves a high shine by reducing the pressure. This is the most time-efficient method.

2-STEP POLISHING SYSTEM

This is the most commonly used polishing system. It contains only two polishers: a medium gritted pre-polisher and a fine-gritted high shine polisher.

52

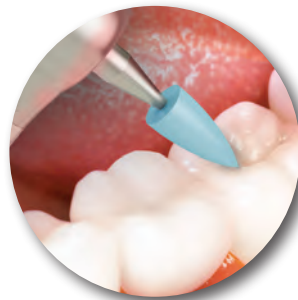

3-STEP POLISHING SYSTEM

The three step polishing system comes with three polishers in different grit sizes.



The first step is to remove excess material and to contour the restoration in preparation for polishing



The second step is to smooth the surface.



The third and final step gives the restoration a high lustre finish.

INSTRUCTIONS FOR USE

These instructions are valid for all KENDA Dental Polishers that are used for restorative and preventive work.

Single-patient polishers are labelled with  and must not be used more than once, as multi-use of these polishers can cause unnecessary risk to the patient and staff.

COMPOSITION:

The polishers consist of synthetic /silicone rubber, pigments and abrasive. The shanks are made of stainless steel or medical plastic.

INDICATION:

KENDA Dental Polishers are used for polishing different materials which are specified on the packaging label.

CONTRAINDICATIONS:

If a patient is known to be allergic to any of the above components, the polishers should not be used.

ADVERSE EFFECT:

None known to date.

GENERAL SECURITY ADVICES:



Do not exceed maximum speed



Wear breathing protection



Wear eye protection



Use waterspray minimum 50ml/min



For polishers with steel shank = 2N plastic shank = 1N

PRECAUTIONS:

- Products may only be used in the specified field of application.
- Check the safe connection of the polisher before using it and perform a test run.
- Use proper hand piece only and remove any damaged , bent, or no longer central running polishers immediately.
- Avoid excessive pressure which can cause tilting, bending or blocking of the polisher.
- Insufficient watercooling can result in irreversible damage to the tooth and the surrounding tissue.

INSTRUCTIONS FOR USE

- Using the wrong disinfectant and/or prolonged disinfection times can soak the polisher or cause discoloration. Therefore, make sure that the effectiveness of the disinfectant is approved and suitable for polishers, do not use disinfectants containing aldehydes and follow the manufacturer's specifications of the product with regard to the concentration and reaction time. Ensure that the process is effective.
- Always keep track of LOT numbers of polishers to ensure traceability.

STORAGE:

A dry, dust-free storage at 2 - 28°C (36 - 82°F) is recommended. Improper storage conditions can shorten the shelf life and cause malfunction of the product.

EXPIRY DATE:

See imprint on label.

HYGIENE INSTRUCTIONS:

Please refer to the following pages for detailed hygiene instructions.

TRANSLATIONS ON [HTTP://KND.LI/INS](http://knd.li/ins)

alb	version shqiptar	ipn	日本語版
ara	النسخة العربية	kor	한국어 버전
bul	българска версия	lav	Latviešu valodā
chi	中國版	lit	Lietuviška versija
cze	Česká verze	mac	македонска верзија
dan	danske version	nor	Norsk versjon
dut	Nederlandse	per	نسخه فارسی
est	Eesti versioon	pol	Polska wersja
fin	Suomalainen versio	por	Versão em português
fre	Version française	rum	Versiunea romana
ger	deutsche Version	rus	Русская версия
gre	Ελληνική έκδοση	slo	slovenská verzia
heb	גרסה עברית	slv	slovenska različica
hrv	hrvatska verzija	spa	Versión en español
hun	magyar változat	swe	Svensk version
ice	Íslensk útgáfa	tur	Türkçe versiyonu
ind	Bahasa Indonesia versi	ukr	Українська версія
ita	Versione italiana		


QR-Code
<http://knd.li/ins>



HYGIENE INSTRUCTIONS

These hygiene instructions are valid for all KENDA Dental Polishers for chairside use.

WARNINGS:

KENDA Polishers are supplied unsterile and therefore must be treated before use. Single patient polishers (labelled with ) are not eligible for reuse, but need to be disinfected and sterilised before and only use.

During processing of all polishers, protective clothing, gloves and goggles must be worn at all times. Only use cleaning and disinfection solutions which are specifically labeled „suitable for silicone or rubber polishers“.

LIMITATION OF REPROCESSING:

The product's life is determined by the wear and tear of the polishing instrument. Repeated processing has minimal effect on these instruments.

POINT OF USE:

Remove surface contamination with a disposable cloth immediately after using on patient and put in a container. Containment and transportation: Polishers should be transported immediately in a closed instrument tray to the treatment area. Proceed with cleaning and disinfection immediately.

CLEANING AND DISINFECTION:

Proceed with either machine (recommended) or manual treatment.

a. Machine treatment:


1. Rinse thoroughly under running water.
2. Place polishers in the washer/disinfector (WD) and make sure they do not touch each other.
3. Add the appropriate cleaning agent (aldehyde-free), according to the information on the product label and the instructions of the WD-manufacturer.
4. Start the desired program: cleaning and disinfection.
5. After termination of the program, take the polishers out of the WD and dry them preferably with clean compressed air.
6. Visual inspection for cleanliness and integrity using a magnifying glass with 6 times magnification. In case of visual contamination, the process must be repeated.
7. If only mechanical cleaning (without proven disinfection) a final disinfection in a steam sterilizer (unpacked) in suitable racks or trays is required.
8. Documented approval of the proper treatment procedure in order to reuse or for storage.
9. A dry, dust-free storage at 2 - 28°C (36 - 82°F) is recommended.

HYGIENE INSTRUCTIONS

b. Manual treatment:

1. Rinse thoroughly under running water. If necessary, use a nylon brush. NOTE: Use a suitable brush for cleaning blind holes.
2. Cleaning and chemical disinfection with a suitable solution (aldehyde-free) according to manufacturer's instruction. Insert polisher into the solution. Make sure that polishers are free of air bubbles.
3. The reaction time begins with the insertion of the last polisher and is according to the instruction of the disinfectant manufacturer.
4. After contact time is up, rinse polishers with plenty of deionized water.
5. Dry residual moisture preferably with clean compressed air.
6. Visual inspection for cleanliness and integrity using a magnifying glass with 6 times magnification. In case of visual contamination, the process must be repeated.
7. Without a proven disinfection, a final disinfection in a steam steriliser (unpacked) in suitable racks or trays is required.
8. Documented approval of the proper treatment procedure in order to reuse or for storage
9. A dry, dust-free storage at 2 - 28°C (36 - 82°F) is recommended.

STERILISATION:



Moist heat sterilisation with fractional prevacuum. Full cycle, 134°C (273°F) /3,1 bar for at least 5 minutes, drying time 10 minutes. Do not exceed 135°C (275°F).

IMPORTANT: Use suitable packaging for sterilisation.

Warning: KENDA Dental Polishers are not suitable for sterilisation with hot air or chemiclave. This procedure was validated by an independent and accredited laboratory.

ADDITIONAL INFORMATION:

When sterilising multiple instruments in one autoclave cycle ensure that the steriliser's maximum load is not exceeded in accordance with the steriliser's instructions.

MANUFACTURER CONTACT:

KENDA AG, Kanalstrasse 18, LI-9490 Vaduz, Liechtenstein.
<http://www.kenda-dental.com>

DATE OF PREPARATION:

10/2016; Rev. 4 The instructions provided above have been validated by the medical device manufacturer as being capable of preparing KENDA Dental Polishers for reuse.

The material has been developed solely for use in dentistry. Processing should be carried out strictly according to the Hygiene Instructions. Liability cannot be accepted for damages resulting from failure to observe the instructions or the stipulated area of application. The user is responsible for testing the products for their suitability and use for any purpose not explicitly stated in the instructions. Descriptions and data constitute no warranty of attributes and are not binding.

KEEP OUT OF REACH OF CHILDREN. FOR USE IN DENTISTRY ONLY.

RX ONLY. Caution: U.S. federal law restricts this device to sale by or on the order of a licensed dentist.



KENDA AG • Dental Manufacturing • Industriezone Neugut
Kanalstrasse 18 • LI-9490 Vaduz • Principality of Liechtenstein

Phone +423 388 23 11 • Fax +423 388 23 19
info@kenda-dental.com • www.kenda-dental.com



© All material herein is copyrighted by KENDA.
Printing is permitted without editing. All editing is prohibited.
Contact us for any questions regarding graphical material.